

TaurineMicroplate Assay Kit User Manual

Catalog # CAK1249

(Version 1.4A)

Detection and Quantification of Taurine Contentin Tissue extracts,
Cell lysate, Cell culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.



I. INTRODUCTION	2
II. KIT COMPONENTS	3
III. MATERIALS REQUIRED BUT NOT PROVIDED	3
IV. SAMPLE PREPARATION	4
V. ASSAY PROCEDURE	5
VI. CALCULATION	6
VII. TYPICAL DATA	7
VIII. TECHNICAL SUPPORT	7
IX NOTES	7



I. INTRODUCTION

Taurine is a sulfur amino acid, an essential amino acid in pre-term and newborn infants of humans and many other species. Taurine is abundant in the brain, heart, breast, gallbladder and kidney and has important roles in health and disease in these organs. Taurine has many diverse biological functions serving as a neurotransmitter in the brain, a stabilizer of cell membranes and a facilitator in the transport of ions such as sodium, potassium, calcium and magnesium. Taurine is highly concentrated in animal and fish protein, which are good sources of dietary taurine. Taurine has many important metabolic roles. Supplements can stimulate prolactin and insulin release.

Taurine Microplate Assay Kit provides a convenient tool for sensitive detection of Taurine in a variety of samples. Taurine reacts with acetylacetone to form a yellow complex. The intensity of the product color, measured at 400 nm, is proportional to the Taurine concentration in the sample.



II.KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer I	30 ml x 3	4 °C
Assay Buffer II	30 ml x 1	4 °C
Dye Reagent A	10 mlx 1	4 °C
Dye Reagent B	0.6 ml x 1	4 °C
Standard	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

Note:

Dye ReagentWorking Solution: add 0.6 ml Dye ReagentBinto Dye ReagentA, mix before use.

Standard: add 1 ml distilled water to dissolve before use; then add 0.5 ml into 0.5 ml distilled water, mix, the concentration will be 10 mmol/L.

III. MATERIALS REQUIRED BUT NOT PROVIDED

- 1. Microplate reader to read absorbance at 400 nm
- 2. Distilled water
- 3. Pipettor, multi-channel pipettor
- 4. Pipette tips
- 5. Mortar
- 6. Centrifuge
- 7. Timer
- 8.Convection oven



IV. SAMPLE PREPARATION

1.For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 0.75mlAssay Buffer I for 5×10^6 cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s,repeat 30 times); then add 0.25mlAssay Buffer II,centrifuged at 10,000g for 10minutes, take the supernatant into a new centrifuge tube for detection.

2.For tissue samples

Weigh0.1 g tissue, homogenize with 0.75mlAssay Buffer I, incubate at 40°Cwater bath for 30 minutes; then add 0.25mlAssay Buffer II, centrifuged at 10,000g for 10minutes, take the supernatant into a new centrifuge tube for detection.

3. For serum or plasma samples

Add 0.75mlAssay Buffer Iinto 0.5 ml samples, mix; centrifuged at 10,000g for 10minutes, take the supernatant into a new centrifuge tube, then add 0.25mlAssay Buffer II, mix.



V. ASSAY PROCEDURE

Add following reagents into the microplate:

Reagent	Sample	Standard	Blank
Sample	100μΙ		
Standard		100μΙ	
Distilled water			100μΙ
Dye ReagentWorking Solution	100 μΙ	100 μΙ	100 μΙ

Mix, cover the plate adhesive strip, put the plate into the convection oven,90°C for 15minutes. When cold, record absorbance measured at 400 nm.

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) The concentrations can vary over a wide range depending on the different samples. For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.
- 3) If any precipitate, please add the samples into the microcentrifuge tube, centrifuged at 10,000g for 10minutes; then add the supernatant into the microplate to read the result.
- 4) Reagents must be added step by step, can not be mixed and added together.



VI. CALCULATION

1. According to the weight of sample

Taurine (
$$\mu$$
mol/g) =(C_{Standard}×V_{Standard})×(OD_{Sample} - OD_{Blank}) / (OD_{Standard} - OD_{Blank}) / (W ×V_{Sample}/ V_{Assay})

=
$$10 \times (OD_{Sample} - OD_{Blank}) / (OD_{Standard} - OD_{Blank}) / W$$

2. According to the quantity of cells or bacteria

Taurine (
$$\mu$$
mol/10⁴)=(C_{Standard}×V_{Standard})×(OD_{Sample} - OD_{Blank}) / (OD_{Standard} - OD_{Blank}) / (N ×V_{Sample}/ V_{Assay})

=
$$10 \times (OD_{Sample} - OD_{Blank}) / (OD_{Standard} - OD_{Blank}) / N$$

3. According to the volume of sample

Taurine (
$$\mu$$
mol/ml)=($C_{Standard} \times V_{Standard}) \times (OD_{Sample} - OD_{Blank}) / (OD_{Standard} - OD_{Blank}) / V_{Sample} \times 3$

 $C_{Standard}$: the concentration of standard, 10mmol/L = 10 μ mol/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria, $N \times 10^4$;

V_{Standard}: the volume of standard, 0.1 ml;


V_{Sample}: the volume of sample, 0.1 ml;

V_{Assav}: the volume of Assay Buffer I and Assay Buffer II, 1 ml.



VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

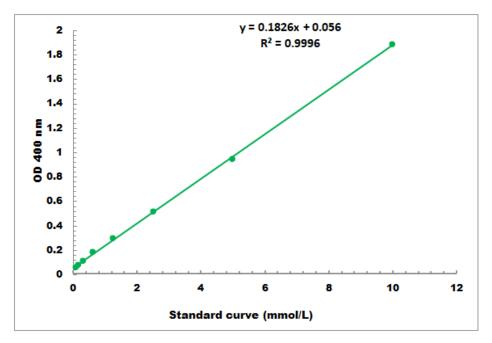

Detection Range: 0.1 mmol/L - 10 mmol/L

VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online towww.cohesionbio.com or contact us at techsupport@cohesionbio.com

IX. NOTES